


Technical Specification

O2-A3 Oxygen Sensor



Figure 1 O2-A3 Schematic Diagram

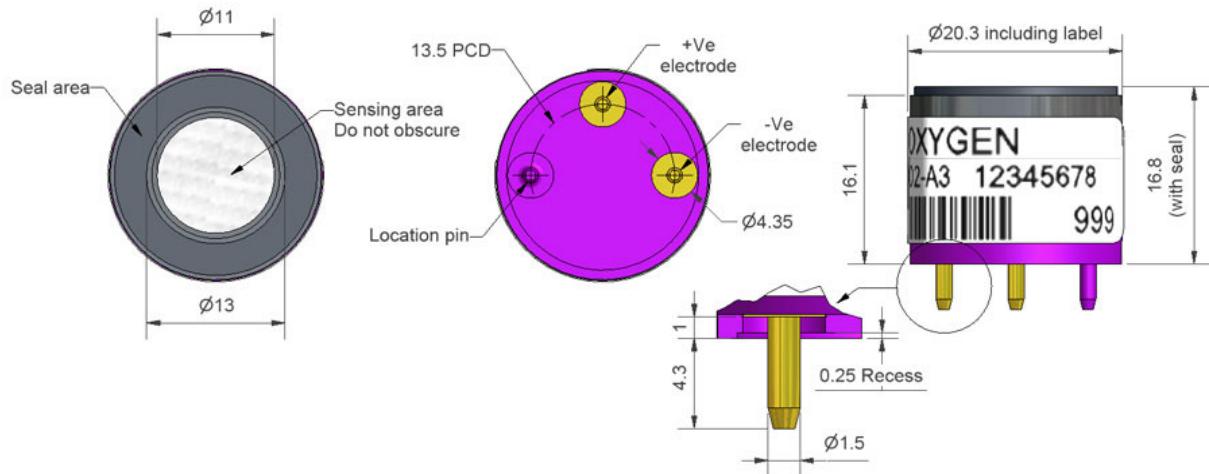

All dimensions in millimetres ($\pm 0.1\text{mm}$)

Top View

Bottom View

Side View

PERFORMANCE	Output Response time Zero current	μA @ 22°C, 20.9% O_2 t_{90} (s) from 20.9% to 0% O_2 (47W load resistor) μA @ 99.99% N_2 , 22°C	65 to 85 < 15 < 2
LIFETIME	Output drift Operating life	% change in output @ 3 months months until 85% original output in 20.9% O_2	< 2 > 36
ENVIRONMENTAL			
	Humidity sensitivity CO_2 sensitivity Pressure sensitivity	% O_2 change: 0% to 95% rh @ 40°C % change in output / % CO_2 @ 5% CO_2 (% change of output)/(% change of pressure) @ 20kPa	< 0.7 + 0.1 < 0.1
KEY SPECIFICATIONS			
	Temperature range Pressure range Humidity range Storage period Load resistor Weight	$^{\circ}\text{C}$ kPa % rh continuous (0 to 99% rh short term) months @ 3 to 20°C (store in sealed container) Ω (recommended) g	-30 to 55 80 to 120 5 to 95 6 47 to 100 <16



NOTE: all sensors are tested at ambient environmental conditions, with 47 ohm load resistor, unless otherwise stated. As applications of use are outside our control, the information provided is given without legal responsibility. Customers should test under their own conditions, to ensure that the sensors are suitable for their own requirements.

Technical Specification

O2-A3 Performance Data

Figure 2 Temperature Dependence in Air

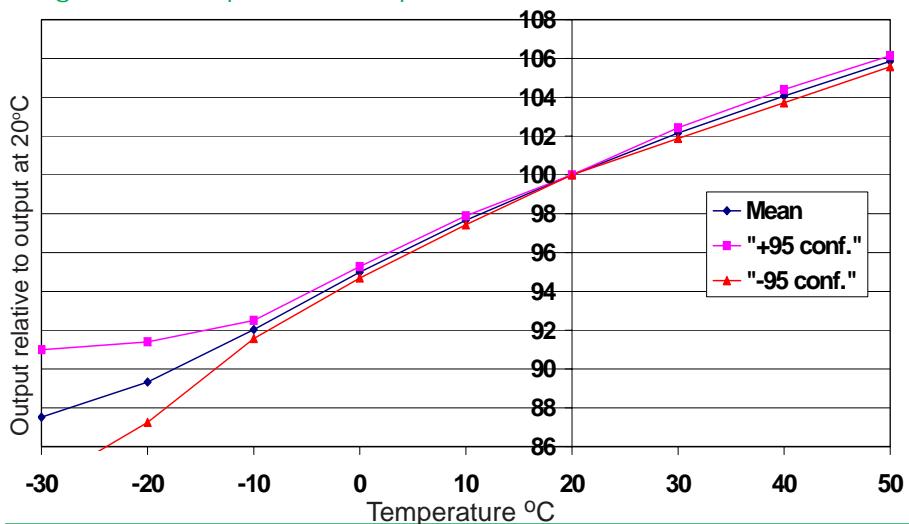


Figure 2 shows the variation of output caused by changes in temperature in 20.9% oxygen. The mean and $\pm 95\%$ confidence intervals are shown.

All capillary oxygen sensors show a change in signal with temperature, and the very repeatable 95% confidence intervals for the O2-A3 are shown.

Figure 3 Pressure Step Performance


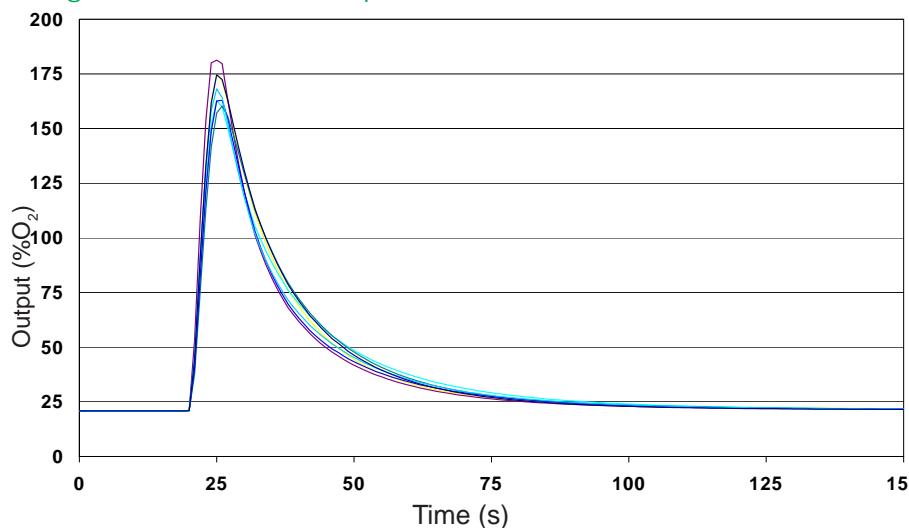


Figure 3 shows how a 25 kPa pressure step change causes a signal transient that decays reproducibly. Negative pressure changes cause a negative transient.

The small shift in final output is less than 10% of the pressure change, so 10kPa pressure step shifts output by less than 1% (<0.2% oxygen).

Figure 4 Long Term Stability

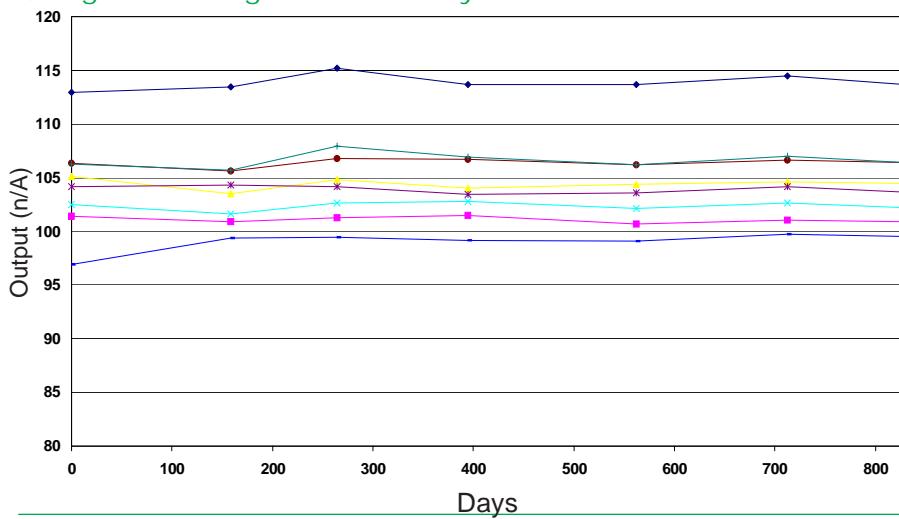

When sensors are rapidly cooled from +20°C to -30°C, sensors perform repeatably without transients or unpredictable output spikes.